



ABLATION PROBE WITH TEMPERATURE SENSITIVE ELECTRODE ARRAY
Robert J. Garabedian, et al
10/734,648

FIG. 1

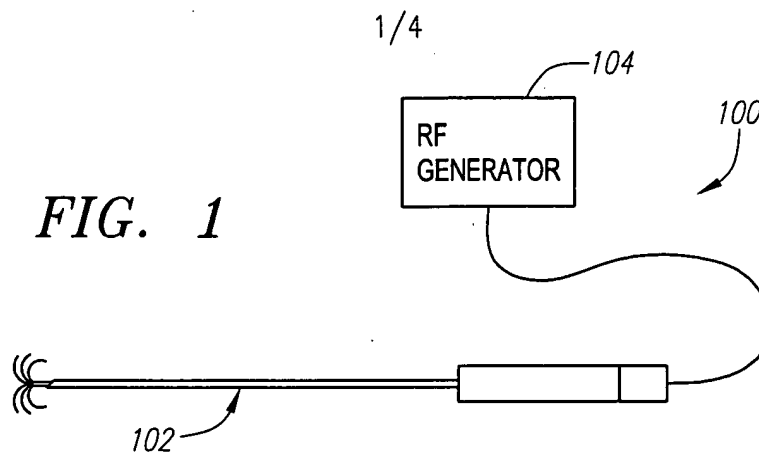


FIG. 2


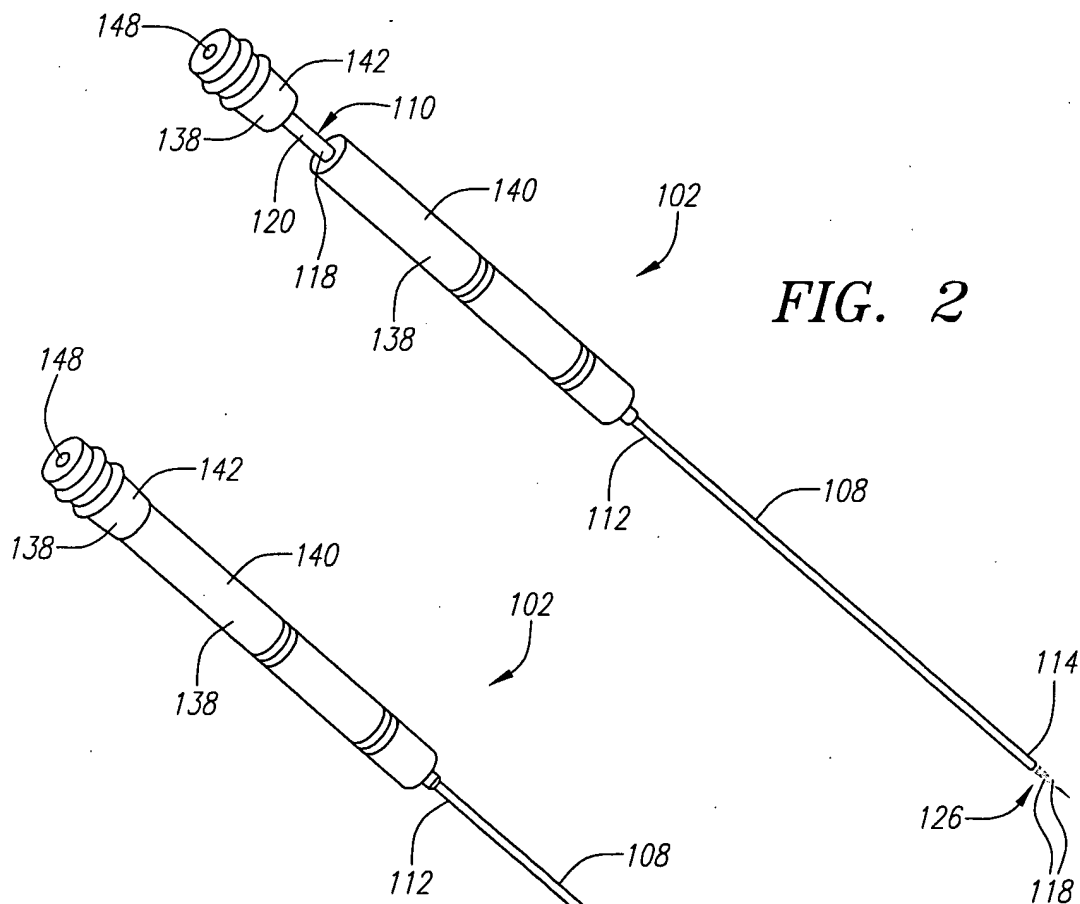


FIG. 3



2/4

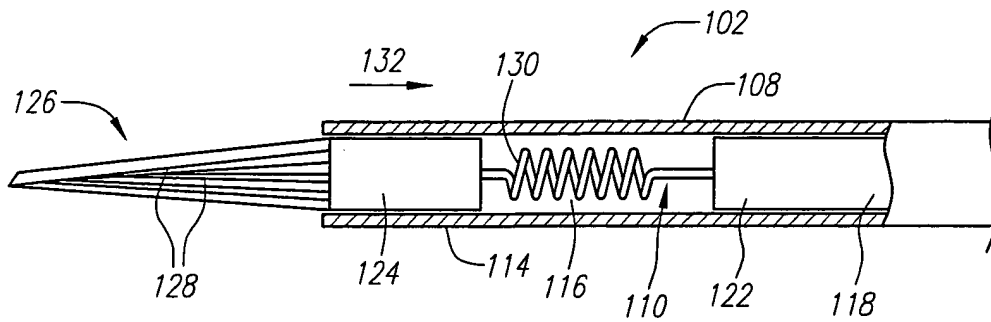


FIG. 4

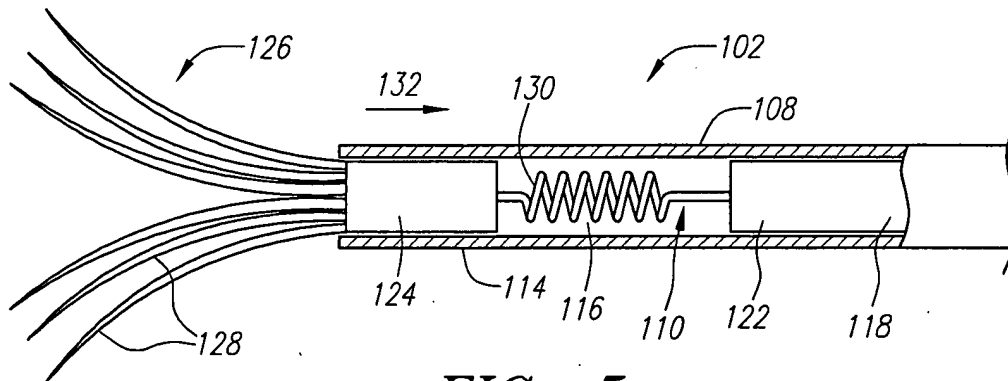


FIG. 5

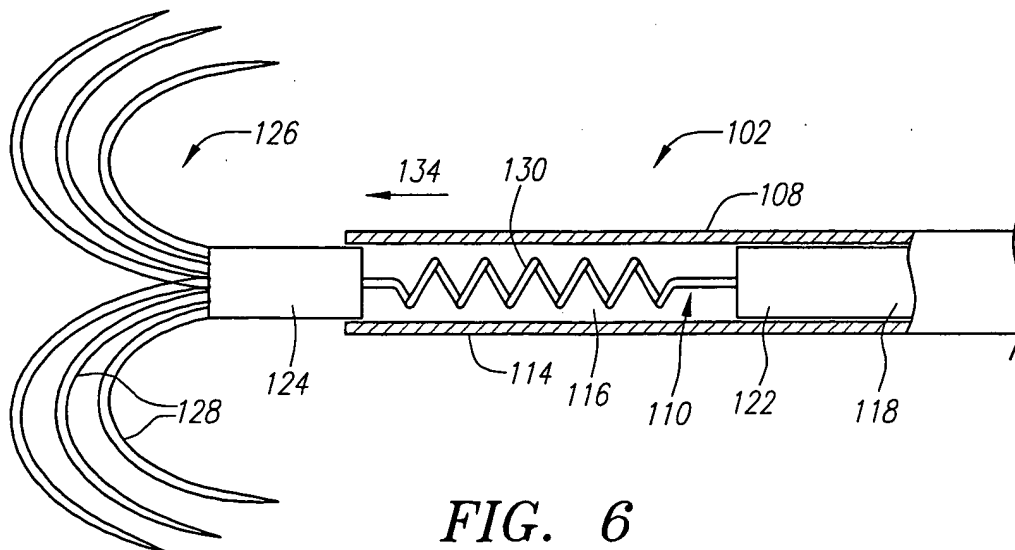


FIG. 6

3/4

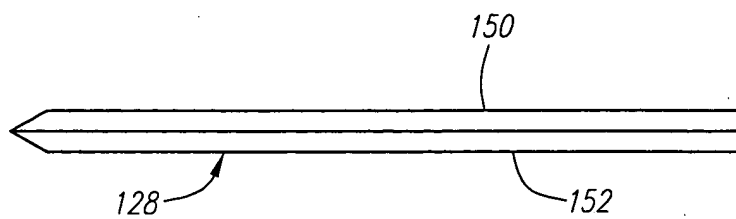


FIG. 7

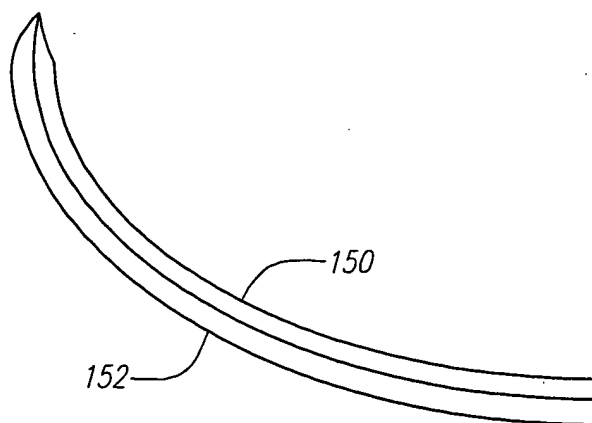


FIG. 8

4/4

FIG. 9A

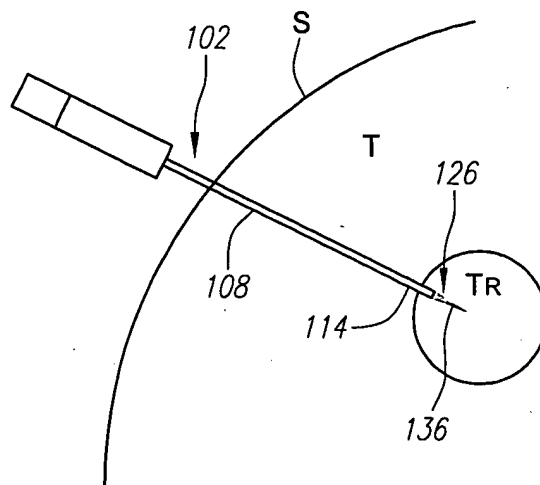


FIG. 9B

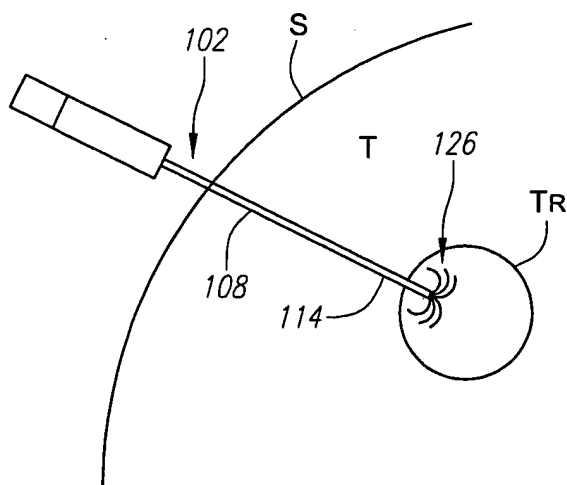


FIG. 9C

